

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: HIGHTSTOWN POLICE
Serial No.: ARTN-0042
Calibration File No.: 01687
Calib. Date: 01/13/2023
Calib. No.: 00046
Certification File No.: 01674
Cert. Date: 09/02/2022
Cert. No.: 00040
Linearity File No.: 01675
Lin. Date: 09/02/2022
Lin. No.: 00040
Solution File No.: 01685
Soln. Date: 01/03/2023
Soln. No.: 00312
Sequential File No.: 01687
File Date: 01/13/2023


Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 21210
Model No.: CU-34
Serial No.: DDUL S3-0183
Expires: 06/16/2023
Bottle No.: 1084

Coordinator

Last Name: GUARCELLO
First Name: COREY
MI: R.

Signature:  Badge No.: 7035
Date: 01/13/2023

*Black Key Temperature Probe Serial.....# DDHH P2 - 055 (8)
*Digital NIST Temperature Measuring System Serial.....# 221 473 070 (8)

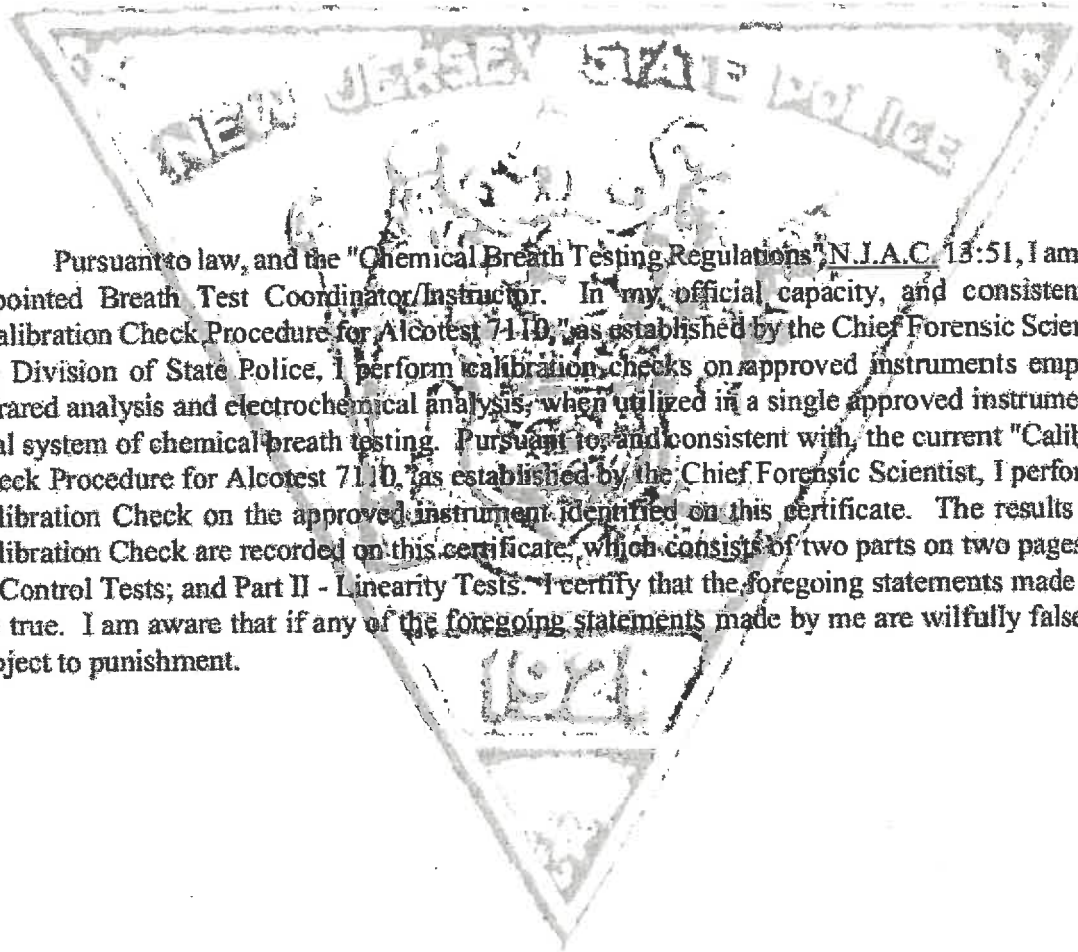

Pursuant to law, and the "Chemical Breath Testing Regulations", N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0042
Location: HIGHTSTOWN POLICE
Calibration File No.: 01687 Calib. Date: 01/13/2023 Calib. No.: 00046
Certification File No.: 01688 Cert. Date: 01/13/2023 Cert. No.: 00041
Linearity File No.: 01675 Lin. Date: 09/02/2022 Lin. No.: 00040
Solution File No.: 01685 Soln. Date: 01/03/2023 Soln. No.: 00312
Sequential File No.: 01688 File Date: 01/13/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0183
Control Solution %: 0.100% Expires: 06/16/2023
Solution Control Lot: 21210 Bottle No.: 1084

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:52S		
Control 1 EC	0.100%	10:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:54S		
Control 2 EC	0.097%	10:54S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:55S		
Control 3 EC	0.099%	10:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:57S		

All tests within acceptable tolerance.

Coordinator

Last Name: GUARCELLO First Name: CORBY MI: R.
Signature:  Badge No.: 7035
Date: 01/13/2023

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTN-0042
Location: HIGHTSTOWN POLICE
Calibration File No.: 01687 Calib. Date: 01/13/2023 Calib. No.: 00046
Certification File No.: 01688 Cert. Date: 01/13/2023 Cert. No.: 00041
Linearity File No.: 01689 Lin. Date: 01/13/2023 Lin. No.: 00041
Solution File No.: 01685 Soln. Date: 01/03/2023 Soln. No.: 00312
Sequential File No.: 01689 File Date: 01/13/2023

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0012
Control Solution %: 0.040% Expires: 07/06/2023
Solution Control Lot: 21250 Bottle No.: 0722

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0012
Control Solution %: 0.080% Expires: 07/19/2023
Solution Control Lot: 21260 Bottle No.: 0760

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0261
Control Solution %: 0.160% Expires: 07/29/2023
Solution Control Lot: 21290 Bottle No.: 0335

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:11S		
Control 1 EC	0.042%	11:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	11:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13S		
Control 2 EC	0.041%	11:14S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	11:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:16S		
Control 3 EC	0.080%	11:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.079%	11:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:18S		
Control 4 EC	0.079%	11:19S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.081%	11:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:21S		
Control 5 EC	0.161%	11:21S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.162%	11:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:23S		
Control 6 EC	0.160%	11:24S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.161%	11:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:26S		

All tests within acceptable tolerance.

Coordinator

Last Name: GUARCELLO

First Name: COREY

MI: R.

Signature: 

Badge No.: 7035

Date: 01/13/2023

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE		
Calibration File No.:	01687	Calib. Date:	01/13/2023
Certification File No.:	01688	Cert. Date:	01/13/2023
Linearity File No.:	01689	Lin. Date:	01/13/2023
Solution File No.:	01690	Soln. Date:	01/13/2023
Sequential File No.:	01690	File Date:	01/13/2023

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0183
Control Solution %:	0.100%			Expires:	05/09/2024
Solution Control Lot:	22160			Bottle No.:	0816

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:33S		
Control 1 EC	0.101%	12:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35S		
Control 2 EC	0.099%	12:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:37S		
Control 3 EC	0.099%	12:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:38S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDWJ P2-055 (CP)

Changed By:

Last Name: GUARCELLO

First Name: COREY

MI: R.

Signature: 

Badge No.: 7035

Date: 01/13/2023

Alcotest 7110 MKIII-C Calibration NIST-Traceable Digital Thermometer Readings

Coordinator:

Tipr Corey R. Guarcello
Name

7035
Badge No.

Location:

Hightstown Police
Agency

ARTN-0042
Alcotest Serial No.

Equipment:

221 473 070
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDRK 53-0012	09:36 S	10:38 S	34.0°C
0.08%	DDSC 53-0012	09:36 S	10:39 S	33.9°C
0.10%	DDUL 53-0183	09:36 S	10:40 S	33.9°C
0.16%	DDWF 53-0261	09:36 S	10:41 S	34.0°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tipr Corey R. Guarcello
Coordinator's Signature

01/13/2023
Date

Dräger
Alcotest® 7110 MDR-C

CERTIFICATE OF ACCURACY

This is a certificate of accuracy for the Alcotest 7110 MDR-C. It is not a guarantee of accuracy. The accuracy of the Alcotest 7110 MDR-C is dependent on the accuracy of the calibration gas and the accuracy of the calibration procedure. The accuracy of the Alcotest 7110 MDR-C is dependent on the accuracy of the calibration gas and the accuracy of the calibration procedure. The accuracy of the Alcotest 7110 MDR-C is dependent on the accuracy of the calibration gas and the accuracy of the calibration procedure.

Calibration Date
3-7-13

SERIAL NUMBER
ARTN-0042

Dräger Safety Engineering, Inc. PC



Calibration complies with ISO/IEC 17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-13326331

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 221473070

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath	93139		
Temperature Probe	128	09 Jul 2022	15-D4F0Q-40-1
Thermistor Module	A17118	08 Jul 2022	1000469276
Temperature Calibration Bath	A45240		
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Thermistor Module	B96381	18 Aug 2022	1000470702
Temperature Probe	5392	04 Aug 2022	4500006080
Temperature Probe	5398	24 Aug 2022	4500006081
Thermistor Module	B96382	08 Oct 2022	1000472708
Temperature Probe	5410	20 Oct 2022	4500006780

Certificate Information:

Technician: 299

Procedure: CAL-06

Cal Date: 25 Apr 2022

Cal Due Date: 25 Apr 2024

Test Conditions: 58.46%RH 23.43°C 1017mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.002	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.000	25.001	Y	24.95	25.05	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.000	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		100.001	99.998	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO Guide to the Expression of Uncertainty in Measurement: (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Marisa Elms
Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2008-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-13326331

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 25 Apr 2022

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2017 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:
DDPKS3-0012

Certification Date:
4.5.22

Technician:
MB

Re-Certification Due Date:
4.5.23



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.


- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:
DDSCS3-0012

Certification Date:
4.5.22

Technician:
MB

Re-Certification Due Date:
4.5.23



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: _____

Serial Number:

DDWFS3-0261

Certification Date:

4.5.22

Technician:

MB

Re-Certification Due Date:

4.5.23

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDHHP2-055

Certification Date:

6.16.22

Next Certification Due:

6.16.23

Probe Value:

104

Dräger, Inc.

MB

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDULS3-0183

Certification Date:

Technician:

Re-Certification Due Date:

9/26/2022

TM/ MB

9/26/2023

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

Certification Date:

Next Certification Due:

DDWJP2-055

9/26/2022

9/26/2023

Probe Value:

103

Dräger, Inc.

TM/ MB



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WLS1 TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/07/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21210

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1199 to 0.1215 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 16, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 07 day of July, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURHIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests; pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 06, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recycled Ink





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/27/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0970 to 0.0977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 19, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recycled Ink





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/11/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21290

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1945 to 0.1977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 29, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 10 day of August, 2021.

Notary signature

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Motor and Public Safety
 This is to certify that

Corey R. Guarcello

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1986 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**

A METHOD TO DETERMINE INTOXICATION GIVEN UNDER MY HAND AT TESTON, NEW JERSEY, THIS 7th DAY OF **December**

TWO THOUSAND AND **Twenty One**

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1		
2		
3		
4		
5		
6		
7		
8		
9		

S.P. 2008 (Rev. 07/21)

DEPARTMENT OF
Motor and Public Safety
 This is to certify that

Corey R. Guarcello
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1986 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**

A METHOD TO DETERMINE INTOXICATION GIVEN UNDER MY HAND AT TESTON, NEW JERSEY, THIS Eleventh DAY OF **November**

TWO THOUSAND AND **Ten**

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1	6-14-12 Means Co PA	C.R.
2	11-13-14 DEERFIELD	C.R.
3	11-21-16 MORRIS Co PA	C.R.
4	2-27-18 BERGEN Co PA	C.R.
5	9/25/20 MORRIS Co PA	C.R.
6	4/8/21 NJCIP	C.R.
7		
8		
9		

S.P. 2008 (Rev. 03/10)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

MATTHEW J. PLATKIN
Acting Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 05/23/2022

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 22160

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is May 9, 2024.


As Acting OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy

Michael Kennedy
OFS Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of May, 2022.

Notary

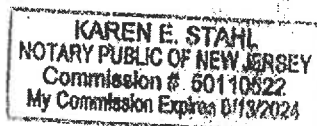

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable

