

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	00901	Calib. Date: 03/14/2013
Certification File No.:	00902	Calib. No.: 00021
Linearity File No.:	00903	Cert. Date: 03/14/2013
Solution File No.:	00912	Cert. No.: 00016
Sequential File No.:	00912	Lin. Date: 03/14/2013
		Lin. No.: 00016
		Soln. Date: 04/29/2013
		Soln. No.: 00153
		File Date: 04/29/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0183
Solution Control Lot:	12II07	Expires: 09/13/2014
		Bottle No.: 0873

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:28D		
Control 1 EC	-.---%	07:29D	N/A	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	07:29D	N/A	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: NIRO

First Name: SGT

MI: J

Signature: \_\_\_\_\_

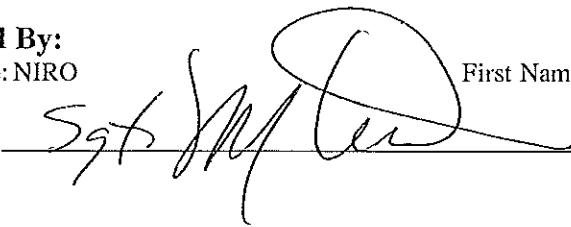

Badge No.: 1114

Date: 04/29/2013