

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	00835	Calib. Date: 08/31/2012
Certification File No.:	00836	Calib. No.: 00019
Linearity File No.:	00837	Cert. Date: 08/31/2012
Solution File No.:	00878	Cert. No.: 00015
Sequential File No.:	00878	Lin. Date: 08/31/2012
		Lin. No.: 00015
		Soln. Date: 01/03/2013
		Soln. No.: 00141
		File Date: 01/03/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0183
Solution Control Lot:	11G093	Expires: 07/07/2013
		Bottle No.: 0896

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:52S		
Control 1 EC	0.100%	20:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:53S		
Control 2 EC	0.098%	20:54S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	20:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:55S		
Control 3 EC	0.099%	20:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NIRO

First Name: SGT

MI: J

Signature: _____

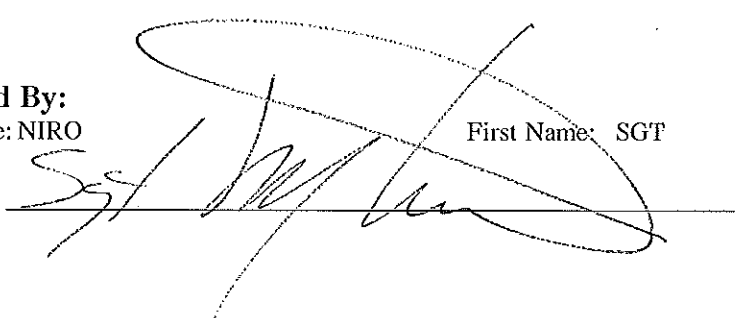

Badge No.: 1114

Date: 01/03/2013