

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE		
Calibration File No.:	00942	Calib. Date:	09/13/2013
Certification File No.:	00943	Cert. No.:	00022
Linearity File No.:	00944	Cert. Date:	09/13/2013
Solution File No.:	00956	Lin. Date:	09/13/2013
Sequential File No.:	00956	Soln. Date:	11/15/2013
		File Date:	11/15/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S3-0182
Solution Control Lot:	12I107	Expires:	09/13/2014
		Bottle No.:	0870

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:16S		
Control 1 EC	0.100%	12:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18S		
Control 2 EC	0.099%	12:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	12:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19S		
Control 3 EC	0.099%	12:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: NIRO

First Name: SGT

MI: J

Signature:

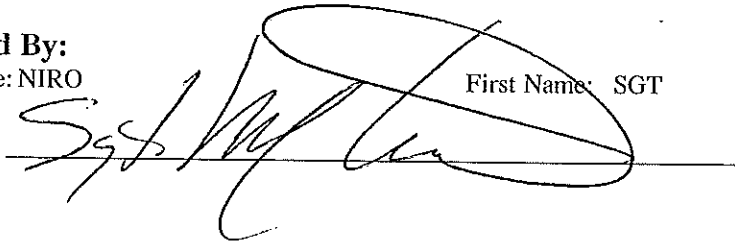

Badge No.: 1114

Date: 11/15/2013