

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	00942	Calib. Date: 09/13/2013
Certification File No.:	00943	Calib. No.: 00022
Linearity File No.:	00944	Cert. Date: 09/13/2013
Solution File No.:	00959	Cert. No.: 00017
Sequential File No.:	00959	Lin. Date: 09/13/2013
		Lin. No.: 00017
		Soln. Date: 12/05/2013
		Soln. No.: 00161
		File Date: 12/05/2013

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0182
Control Solution %:	0.100%		Expires: 09/13/2014
Solution Control Lot:	12I107		Bottle No.: 0875

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	21:04S		
Control 1 EC	0.099%	21:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	21:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:05S		
Control 2 EC	0.098%	21:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	21:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:07S		
Control 3 EC	0.099%	21:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	21:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:08S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NIRO

First Name: SGT

MI: J

Signature: _____

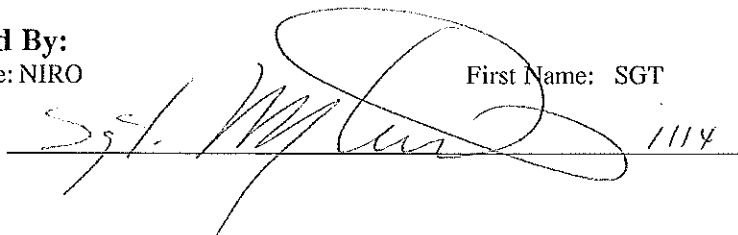

Badge No.: 1114

Date: 12/05/2013