

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTN-0042  
**Location:** HIGHTSTOWN POLICE  
**Calibration File No.:** 00835 **Calib. Date:** 08/31/2012 **Calib. No.:** 00019  
**Certification File No.:** 00836 **Cert. Date:** 08/31/2012 **Cert. No.:** 00015  
**Linearity File No.:** 00837 **Lin. Date:** 08/31/2012 **Lin. No.:** 00015  
**Solution File No.:** 00895 **Soln. Date:** 02/10/2013 **Soln. No.:** 00148  
**Sequential File No.:** 00895 **File Date:** 02/10/2013

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUL S3-0183  
**Control Solution %:** 0.100% **Expires:** 07/07/2013  
**Solution Control Lot:** 11G093 **Bottle No.:** 0876

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:05S		
Control 1 EC	0.100%	10:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		
Control 2 EC	0.098%	10:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08S		
Control 3 EC	0.098%	10:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:10S		

All tests within acceptable tolerance.

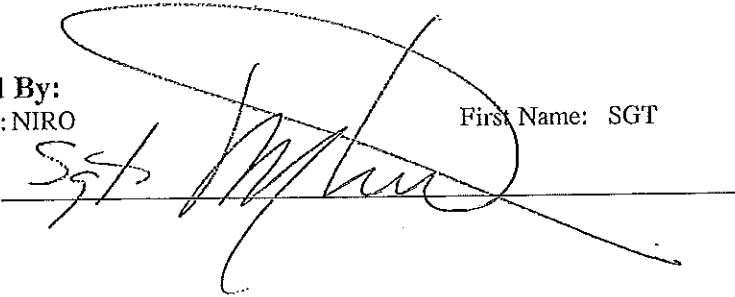
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: NIRO

First Name: SGT

MI: J

Signature: 

Badge No.: 1114

Date: 02/10/2013