

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTN-0042
Location:	HIGHTSTOWN POLICE		
Calibration File No.:	01167	Calib. Date:	01/11/2016
Certification File No.:	01168	Cert. No.:	00028
Linearity File No.:	01169	Cert. Date:	01/11/2016
Solution File No.:	01205	Lin. No.:	00023
Sequential File No.:	01205	Lin. Date:	01/11/2016
		Soln. No.:	00204
		Soln. Date:	04/27/2016
		File Date:	04/27/2016

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUL S3-0183
Control Solution %:	0.100%			Expires:	03/22/2018
Solution Control Lot:	201603L			Bottle No.:	1450

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:37D		
Control 1 EC	0.102%	15:38D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	15:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:38D		
Control 2 EC	0.101%	15:39D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	15:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:40D		
Control 3 EC	0.101%	15:41D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	15:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:41D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: GENDRON

First Name: FRANK

MI: G

Signature: \_\_\_\_\_

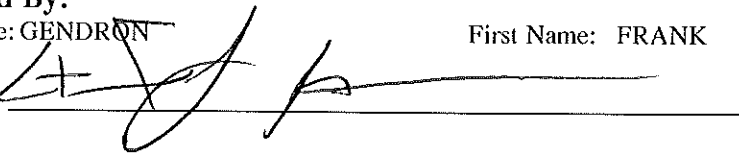

Badge No.: 1120

Date: 04/27/2016