

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	01318	Calib. Date: 01/08/2018
Certification File No.:	01319	Calib. No.: 00033
Linearity File No.:	01320	Cert. Date: 01/08/2018
Solution File No.:	01348	Cert. No.: 00028
Sequential File No.:	01348	Lin. Date: 01/08/2018
		Lin. No.: 00028
		Soln. Date: 03/19/2018
		Soln. No.: 00233
		File Date: 03/19/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0183
Solution Control Lot:	17290	Expires: 09/14/2019
		Bottle No.: 0738

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:17S		
Control 1 EC	0.101%	12:18S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:18S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19S		
Control 2 EC	0.100%	12:20S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	12:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21S		
Control 3 EC	0.101%	12:21S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22S		

All tests within acceptable tolerance.

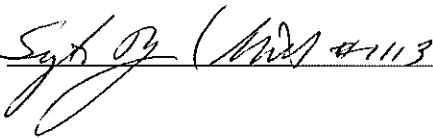
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MILLER

First Name: BENJAMIN

MI: L

Signature:  #1113

Badge No.: 1113

Date: 03/19/2018