

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARTN-0042
Location:	HIGHTSTOWN POLICE	
Calibration File No.:	01524	Calib. Date: 07/23/2020
Certification File No.:	01525	Calib. No.: 00039
Linearity File No.:	01526	Cert. Date: 07/23/2020
Solution File No.:	01543	Cert. No.: 00034
Sequential File No.:	01543	Lin. Date: 07/23/2020
		Lin. No.: 00034
		Soln. Date: 11/19/2020
		Soln. No.: 00277
		File Date: 11/19/2020

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUL S3-0183
Control Solution %:	0.100%		Expires: 07/06/2022
Solution Control Lot:	20320		Bottle No.: 1346

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:28S		
Control 1 EC	0.100%	14:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:29S		
Control 2 EC	0.099%	14:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:31S		
Control 3 EC	0.100%	14:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MILLER

First Name: BENJAMIN

MI: L

Signature: \_\_\_\_\_

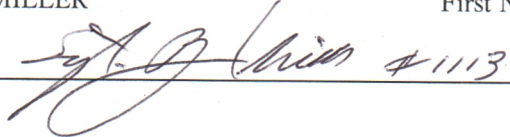

Badge No.: 1113

Date: 11/19/2020